


»» Passion for  
Precision ««

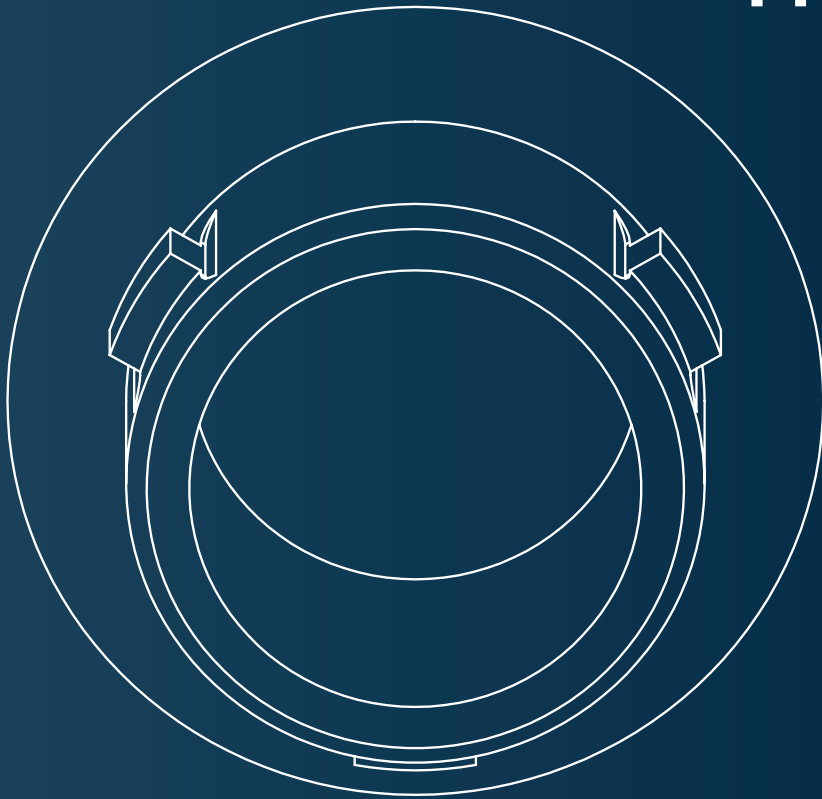

MPS

MULTI PLATFORM SYSTEMS

**NEOSS<sup>®</sup> ProActive<sup>®</sup>**  
**NE-Series**


# NEOSS®

**NE-Serie** We are extending our extensive range with an additional compatible implant interface: ProActive® of NEOSS®.

Medentika® represents continuous further development based on the latest Knowledge in implantology.

We are Made in Germany – We are Medentika®.

Manufacturer	Implant system	compatibel with
NEOSS®	ProActive®*	NE-Series



Implant connection:  
SP D 3,5-6,5

## Portfolio Overview

Laboratory implant  
Scanbody  
Titanium base ASC Flex  
PreFace abutment  
Ti-Forms abutment  
Multi-unit abutment (available august 2021)  
MedentiLOC abutment  
Novaloc abutment  
Optiloc abutment  
Placement instrument

Medentika®  
**NE-Series**

Product Overview



\*is a registered trademark of an independent third party

## Laboratory implant

- Titanium Grade 5 CF



Implant connection	SP D 3,5-6,5	SP D 3,5-6,5
Type		CADCAM
Placement instrument		NE 80 T
Article No.	NE 50	NE 80

## Placement instrument laboratory implant CADCAM

- Stainless steel



Implant connection	SP D 3,5-6,5
Article No.	NE 80 T

## Abutment screw

- Titanium Grade 5 CF



Placement instrument	NEO	Ball Torx
Article No.	NE 60	NE 61

**Please note:** The correct choice of the abutment screw is stated with the respective abutment in the catalogue.

## Laboratory screw

- red coated



Article No.	NE 60 L	NE 61 L
-------------	---------	---------

**Please note:** The correct choice of the laboratory screw is stated with the respective abutment in the catalogue.

## Scanbody

- Titanium
- specially coated
- incl. retention screw



Implant connection	SP D 3,5-6,5
Retention screw	NE 60 SB
Article No.	NE 1400-L

**Please note:** The Scanbody is sterilisable and for intra-oral scanning.

## Titanium base ASC Flex

- angled screw channel
- Titanium Grade 5 CF
- incl. abutment screw
- Type SF = Screw channel angled over the flat of the scanbody Type
- Recommended torque: 32 Ncm




Implant connection	SP D 3,5-6,5	SP D 3,5-6,5
Chimney height	3,5-6,5	3,5-6,5
Gingiva height	0,35 mm	2,5 mm
Placement instrument	Ball Torx	Ball Torx
Abutment screw	NE 61	NE 61
Article No. Type 2/SF	NE 1600-2-SF	NE 1700-2-SF

**Please note:** To screw in the titanium base ASC Flex you need the Placement instrument Ball-Torx M 03-8, M 10-8 or 6-13-06. To select the desired direction of the angled screw channel, please consider the Instruction for use.

## Modelling cap set

- Burn-out plastic
- Scope of Delivery: four chimney heights



Modelling cap set straight	6-09-11	6-09-11
Modelling cap set angled	6-09-12	6-09-12

## Titanium base ASC Flex rotating

- angled screw channel
- Titanium Grade 5 CF
- incl. abutment screw
- Recommended torque: 32 Ncm




Implant connection	SP D 3,5-6,5
Chimney height	3,5-6,5
Gingiva height	0,35 mm
Placement instrument	Ball Torx
Abutment screw	NE 61
Article No.	<b>NE 1800</b>

**Please note:** To screw in the titanium base ASC Flex you need the Placement instrument Ball-Torx M 03-8, M 10-8 or 6-13-06.

## Modelling cap set

- Burn-out plastic
- Scope of Delivery: four chimney heights



Modelling cap set straight	<b>6-09-11</b>
Modelling cap set angled	<b>6-09-12</b>

## PreFace abutment Titanium Grade 5 CF

- incl. abutment screw
- Recommended torque: 32 Ncm



Implant connection	SP D 3,5-6,5
Diameter	11,5 mm
Placement instrument	NEO
Abutment screw	NE 60
Laboratory screw	NE 60 L
Article No.	<b>NE 9000-R</b>

## PreFace abutment CrCo alloy / CTE 14.1

- WAK 14,1
- incl. abutment screw
- Recommended torque: 32 Ncm



Implant connection	SP D 3,5-6,5
Diameter	11,5 mm
Placement instrument	NEO
Abutment screw	NE 60
Laboratory screw	NE 60 L
Article No.	<b>NE 9800-R</b>

## TI-Forms abutment for M-Series

- Titanium Grade 5 CF
- incl. abutment screw
- Recommended torque: 32 Ncm



Implant connection	SP D 3,5-6,5
Diameter	11,5 mm
Placement instrument	NEO
Abutment screw	NE 60
Laboratory screw	NE 60 L
Article No.	<b>NE 9000-ST</b>

## Multi-unit abutment straight

Available August 2021

- Titanium Grade 5 CF
- Sterile packaged
- Recommended torque: 32 Ncm



Implant connection	SP D 3,5-6,5	SP D 3,5-6,5	SP D 3,5-6,5
Gingiva height	1,5 mm	3,5 mm	5,5 mm
Placement instrument	M 11-11	M 11-11	M 11-11
Article No.	<b>NE 8000</b>	<b>NE 8001</b>	<b>NE 8002</b>

**Please note:** To screw in the Multi-unit abutments straight To screw in the Placement instrument M 11-11.

## Multi-unit abutment angled 17°

Available August 2021

- Titanium Grade 5 CF
- Sterile packaged
- incl. abutment screw
- Type 1 = angled over flat
- Recommended torque: 32 Ncm



Implant connection	SP D 3,5-6,5	SP D 3,5-6,5	SP D 3,5-6,5
Gingiva height (mm)	1,1/2,5	2,1/3,5	4,1/5,5
Placement instrument	NEO	NEO	NEO
Abutment screw	NE 60	NE 60	NE 60
Article No.	<b>NE 8100</b>	<b>NE 8101</b>	<b>NE 8102</b>

## Multi-unit abutment angled 30°

Available August 2021

- Titanium Grade 5 CF
- Sterile packaged
- incl. abutment screw
- Type 1 = angled over flat
- Recommended torque: 32 Ncm



Implant connection	SP D 3,5-6,5	SP D 3,5-6,5	SP D 3,5-6,5
Gingiva height (mm)	0,6/3,0	1,6/4,0	3,1/5,5
Placement instrument	NEO	NEO	NEO
Abutment screw	NE 60	NE 60	NE 60
Article No.	NE 8300	NE 8301	NE 8302

## Multi-unit bridge screw

Available August 2021

- Titanium Grade 5 CF
- Recommended torque: 15 Ncm



Placement instrument	Ball Torx	Ball Torx
Article No.	6-31-01	NE 8501

## Multi-unit Prosthetic components

Available August 2021

- Recommended torque: 15 Ncm
- Titanium base / Titanium cap: incl. bridge screw
- Material: Titanium Grade 5 CF
- Modelling sleeve: without bridge screw
- Material: Tecanat (PC)



Description	Titanium base ASC	Titanium base	Titanium cap Flex	Modelling sleeve
Placement instrument	Ball Torx	NEO	NEO	
Screw	6-31-01	NE 8501	NE 8501	
Article No.	6-31-02	NE 8508	NE 8519	8510

Please note: The Multi-unit modelling sleeve can be used with the Multi-unit titanium base and Multi-unit titanium cap.

## Multi-unit Prosthetic components

Available August 2021

- incl. bridge screw
- Recommended torque: 15 Ncm
- Material Gold cap, castable: "(Au 60%; Pd 20%; Pt 19%; Ir 1%)"
- Material CoCr cap: CrCo alloy / CTE 14.1



Description	Gold cap, castable	CoCr cap
Placement instrument	NEO	NEO
Screw	NE 8501	NE 8501
Article No.	NE 8506	NE 8507

## Multi-unit Screw matrix

Available August 2021

- Titanium Grade 5 CF
- Recommended torque: 15 Ncm



Description	MedentiLOC	Novaloc
Placement instrument	NEO	NEO
Article No.	NE 8517	NE 8518

## Multi-unit Scanbody

Available August 2021

- Titanium specially coated
- incl. bridge screw



Version	straight	angled
Placement instrument	NEO	NEO
Screw	NE 8501	NE 8501
Article No.	NE 8500	NE 8513

Please note: The Scanbody is sterilisable and for intra-oral scanning.

## Multi-unit Laboratory implant

Available August 2021

- Titanium Grade 5 CF



Version	straight	angled	angled
Type		17°	30°
Article No.	8504	8514-17	8514-30

## Multi-unit Laboratory implant CAD/CAM

Available August 2021





- Titanium Grade 5 CF



Version	straight	angled	angled
Type		17°	30°
Placement instrument	M 11-11	8515 T	8515 T
Article No.	8509	8515-17	8515-30






## Multi-unit accessories

- NE 8502 Multi-unit cover cap NEO
- NE 8503 Multi-unit Implant pickup incl. retention screw
- M 11-11 Placement
- instrument Multi-unit abutment manual and ratchet
- 8515 T Placement instrument laboratory implant CAD/CAM Multiunit

<b>Description</b>				
	cover cap	implant pickup	Placement instrument	Placement instrument laboratory implant
<b>Article No.</b>	<b>NE 8502</b>	<b>NE 8503</b>	<b>M 11-11</b>	<b>8515 T</b>



## MedentiLOC abutment straight

- Titanium Grade 5 CF
- TiN coated
- Recommended torque: 32 Ncm

					
<b>Implant connection</b>	SP D 3,5-6,5	SP D 3,5-6,5	SP D 3,5-6,5	SP D 3,5-6,5	SP D 3,5-6,5
<b>Gingiva height</b>	1,0 mm	2,0 mm	3,0 mm	4,0 mm	5,0 mm
<b>Placement instrument</b>	Hex 1,26	Hex 1,26	Hex 1,26	Hex 1,26	Hex 1,26
<b>Article No.</b>	<b>NE 2000</b>	<b>NE 2100</b>	<b>NE 2200</b>	<b>NE 2300</b>	<b>NE 2400</b>
<b>Please note:</b>	To screw in the straight MedentiLOC abutments you need the Placement instrument hex 1,26 mm M 03-1 or M 10-1 / M 09-1 or M 11-1.				

## Novaloc® Processing package

- Matrix housing Titanium/PEEK
- Retention insert white Retention force: light
- Retention insert yellow Retention force: medium
- Retention insert green Retention force: strong
- Mounting collar Silocone
- 2 pcs per package
- incl. mounting insert

		
<b>Material Matrix housing</b>	Titanium	PEEK
<b>Article No.</b>	<b>2010.601</b>	<b>2010.611</b>






## MedentiLOC Laboratory implant

- Stainless steel

	
<b>Version</b>	straight
<b>Article No.</b>	<b>56</b>



## Novaloc abutment straight

- Titanium Grade 5 CF
- ADLC coated
- Recommended torque: 32 Ncm

					
<b>Implant connection</b>	SP D 3,5-6,5	SP D 3,5-6,5	SP D 3,5-6,5	SP D 3,5-6,5	SP D 3,5-6,5
<b>Gingiva height</b>	1,0 mm	2,0 mm	3,0 mm	4,0 mm	5,0 mm
<b>Placement instrument</b>	NEO	NEO	NEO	NEO	NEO
<b>Article No.</b>	<b>NE 6000</b>	<b>NE 6100</b>	<b>NE 6200</b>	<b>NE 6300</b>	<b>NE 6400</b>
<b>Please note:</b>	To screw in the straight Novaloc abutments you need the original Placement instrument of the respective series.				

## Novaloc® Processing package

- Matrix housing Titanium/PEEK
- Retention insert white Retention force: light
- Retention insert yellow Retention force: medium
- Retention insert green Retention force: strong
- Mounting collar silocone
- 2 pcs per package
- incl. mounting insert

		
<b>Material Matrix housing</b>	Titanium	PEEK
<b>Article No.</b>	<b>2010.601</b>	<b>2010.611</b>






## Novaloc Laboratory implant

- Stainless steel

	
<b>Version</b>	straight
<b>Article No.</b>	<b>58</b>

## Optiloc abutment straight

- Titanium Grade 5 CF
- ADLC coated
- Recommended torque: 32 Ncm

					
<b>Implant connection</b>	SP D 3,5-6,5	SP D 3,5-6,5	SP D 3,5-6,5	SP D 3,5-6,5	SP D 3,5-6,5
<b>Gingiva height</b>	1,0 mm	2,0 mm	3,0 mm	4,0 mm	5,0 mm
<b>Placement instrument</b>	M 59 / M 79	M 59 / M 79	M 59 / M 79	M 59 / M 79	M 59 / M 79
<b>Article No.</b>	<b>NE 5000</b>	<b>NE 5100</b>	<b>NE 5200</b>	<b>NE 5300</b>	<b>NE 5400</b>
<b>Please note:</b>	To screw in the straight Optiloc abutments you need the special Placement instrument M 59 / M 79.				

## Optiloc® Processing package

- Matrix housing Titanium
- Retention insert white  
Retention force: light
- Retention insert yellow  
Retention force: medium
- Retention insert green  
Retention force: strong
- Mounting collar silicone
- 2 pcs per package



Titanium

**Material**  
**Matrix housing**  
**Article No.**

**5202.0001**

## Placement instrument Optiloc abutment

- Hardened Stainless steel



**Version**

Manual and ratchet    Contra-angle

**Article No.**

**M 59                      M 79**

## Optiloc implant analogue

- Aluminium



**Version**

4 piece

**Article No.**

**2102.0024**

## Placement instrument NEO

- Hardened Stainless steel



**Version**

Contra-angle    Contra-angle    Manual and ratchet    Manual and ratchet

long                      short                      long                      short

**Article No.**

**M 03-12                      M 09-12                      M 10-12                      M 11-12**

18,00 EUR                      18,00 EUR                      34,00 EUR                      34,00 EUR



**Publisher**

Medentika® GmbH

As at: March 2021

We are certified:

**DIN EN ISO 13485**

**Medical Devices Directive 93/42/EEC,  
Annex II**


**CE0483**

The electronic Instructions for Use for our products are available on the website [www.medentika.com](http://www.medentika.com).

# We have a passion for precision, quality and durability

- One of the leading compatibles manufacturer
- Made in Germany
- Compatible with all major implant systems at an affordable price
- Committed to collaboration, teamwork and partnership
- Guaranteed up to lifetime

»» Passion for  
Precision ««

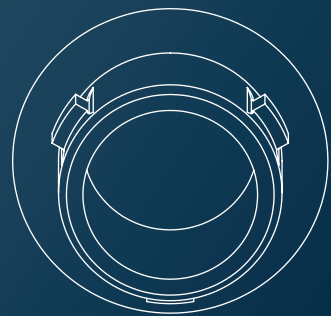

## HERSTELLER

Medentika® GmbH  
Hammweg 8–10  
76549 Hügelshheim  
info@medentika.de  
www.medentika.com

© Medentika® GmbH, 2020. All rights reserved.  
Medentika® and/or other trademarks and logos from Medentika® mentioned herein are the trademarks or registered trademarks of Medentika® and/or its affiliates.

 **MEDENTIKA®**  
A Straumann Group Brand