

Did you know?

22%



of the Canadian population (60 to 79) are edentulous<sup>1</sup>

What do these patients need?

Edentulous patients presenting reduced horizontal bone availability seeking a trustful, affordable stabilization of their overdentures.



Quality of life



Affordability




Reliability



Convenience

How can you meet these demands?

WITH THE STRAUMANN® MINI IMPLANT SYSTEM.

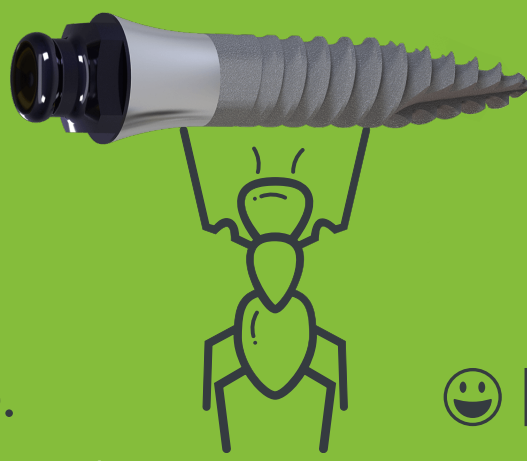

It's affordable.

- Less expensive than regular implants
- Fewer visits and chair time needed



It's convenient.

- Minimally invasive procedures\*
- Designed for immediate loading\*\*

\*If GBR can be avoided  
\*\*If 35Ncm of torque is achieved on all implants



It's reliable.

ROXOLID®

- High material strength<sup>2</sup> and biocompatibility<sup>3</sup>

SLA®

- Scientific evidence<sup>2-8</sup>
- Bone preservation<sup>3-4</sup>

OPTILOC®

- Excellence wear resistance
- Exceptional long term performance

It's designed to trust!



Roxolid®

- proven quality -

Straumann® Mini Implants have a **35% increased fatigue strength<sup>9</sup>** compared to competitive mini implants.



35%

increased STRENGTH



SLA®

- Straumann's Trusted Surface -

- Predictability in osseointegration<sup>2-8</sup>
- Scientific evidence<sup>2-8</sup>
- Low prevalence of peri-implantitis<sup>3</sup>
- Bone preservation<sup>3,4</sup>



Optiloc®

- durability & efficiency -

- Space-saving design
- Reduced maintenance
- ADLC in combination with PEEK: excellence wear resistance

Even a reason more to trust:

Straumann® Mini Implant is backed by our **lifetime limited warranty**



Straumann® Mini Implant System

Learn more:  
[straumann.ca/mini-implant](http://straumann.ca/mini-implant)

LOCK IN THE RIGHT FIT.



REFERENCES

1. <https://www.ncbi.nlm.nih.gov/pmc/articles/PMC3664508/#:~:text=In%202010%2C%20the%20overall%20rate,different%20regions%20within%20a%20country.> 2. Norm ASTM F67 (states min. tensile strength of annealed titanium). 3. <http://www.straumann.com/science-roxolid.html>. 4. Fischer K, Stenberg T. Prospective 10-year cohort study based on a randomized controlled trial (RCT) on implant-supported full-arch maxillary prostheses. Part 1: sandblasted and acid-etched implants and mucosal tissue. Clin Implant Dent Relat Res. 2012 Dec;14(6):808-15. 5. van Velzen FJ, Ofec R, Schulten EA, Ten Bruggenkate CM. 10-year survival rate and the incidence of peri-implant disease of 374 titanium dental implants with an SLA surface: a prospective cohort study in 177 fully and partially edentulous patients. Clin Oral Implants Res. 2015 Oct;26(10):1121-8. 6. Cochran DL, Jackson JM, Bernard JP, ten Bruggenkate CM, Buser D, Taylor TD, Weingart D, Schoolfield JD, Jones AA, Oates TW Jr. A 5-year prospective multicenter study of early loaded titanium implants with a sandblasted and acid-etched surface. Int J Oral Maxillofac Implants. 2011 Nov-Dec;26(6):1324-32. 7. Cochran D, Oates T, Morton D, Jones A, Buser D, Peters F. Clinical field trial examining an implant with a sand-blasted, acid-etched surface. J Periodontol. 2007 Jun;78(6):974-82. 8. Bornstein MM, Schmid B, Belser UC, Lussi A, Buser D. Early loading of non-submerged titanium implants with a sandblasted and acid-etched surface. 5-year results of a prospective study in partially edentulous patients. Clin Oral Implants Res. 2005 Dec;16(6):631-8. 9. Source: data on file, according to ISO 14801, conditions 2016.