


JUVORA™ PEEK

High performance polymer manufactured by JUVORA™



Strong and lightweight high performance polymer indicated for final full-arch restorations

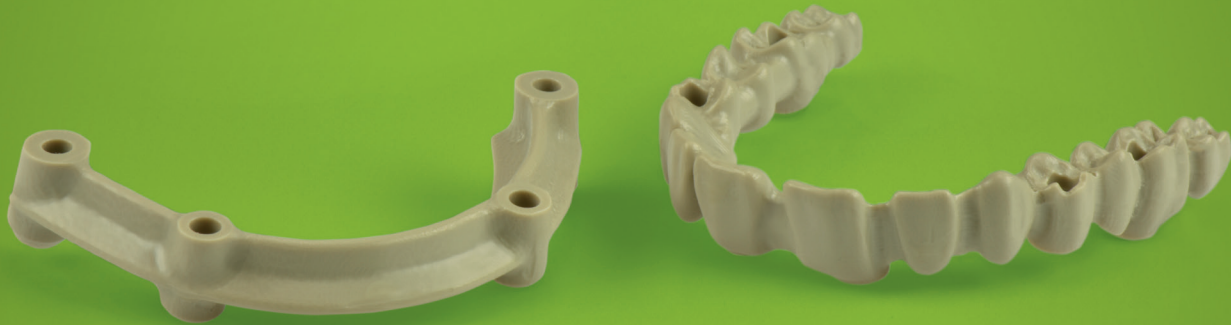

LIGHTWEIGHT

JUVORA™ PEEK is a lightweight alternative to traditional metal frameworks



FLEXIBILITY

The material is steam sterilizable and highly biocompatible providing high flexibility to dental professionals




ENDURANCE

JUVORA™ PEEK is strong and durable, indicated for up to final full-arch restorations

Available shades

► JUVORA™ PEEK restorations (available through our CARES® centralized milling solution) and discs (for in-house milling) are available in two shades: Natural and Oyster White

JUVORA™ PEEK DISC WITH Ø 98 mm (EACH ARTICLE CONTAINS 1 DISC)











Shade	Disc height 16 mm	Disc height 20 mm
 Natural	540001	540005

Available indications






► For final restorations

Recommended indication
Possible indication
Not possible indication (n/a)

TOOTH-BASED

 [n/a] Inlay	 [n/a] Onlay	 [n/a] Veneer	 [n/a] Partial crown	 Coping
 Full-contour crown	 Telescopic crown	 Bridge/bar framework	 Full-contour bridge/bar*	 Vestibular veneering

ABUTMENT-BASED (AVAILABLE WITHIN THE CARES® X-STREAM™ SOLUTION)

				
Bridge/bar framework on Ti-Base Coping for SRA*				
 Coping on CADCAM abutment	 Full-contour crown on CADCAM abutment	 Bridge/bar framework on CADCAM abutments	 Full-contour bridge on CADCAM abutments*	

*Only up to 3 units posterior

Workflow

STEPS	OPTIONS
Nesting	Only for in-house milling
Milling*	Only for in-house milling
Finishing*	Polishing Wrap around (for fixed bars) Layering (with composite veneering only)
Cementing*	Self-adhesive <i>Recommendation:</i> 3M™ RelyX™ Unicem

*For detailed information on the use and handling of JUVORA™ PEEK, please refer to the JUVORA™ processing guide

Chemical composition

ELEMENTS	WEIGHT
Polyetheretherketone (PEEK)	≥ 90.0 %
TiO ₂	≤ 10.0 %

Physical properties

PROPERTIES	VALUE
Density [g/cm ³]	1.3 ± 0.1
Flexural strength [MPa]*	165 ± 10
Melting point [°C]	343
Water absorption [µg/mm ³]*	5 ± 1

*According to ISO 20795


Preparation guidelines

- ▶ The preparation shall not have angles or sharp edges
- ▶ The shoulder preparation shall be with rounded inner edges and/or chamfer


Wall thickness

- ▶ The cross-sections shall be adjusted in relation to the total size of the restoration
- ▶ The transition from a connector to a crown or coping shall be rounded

MINIMAL RESTORATION DESIGN



Restoration wall thickness

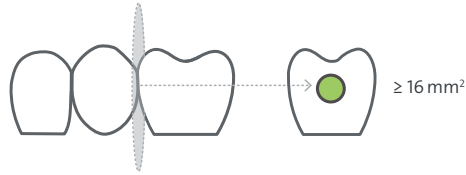

Connector cross-section

Sterilization

- ▶ For restorations bonded to abutments before being placed in the patient's mouth, the product must be sterilized before use. Sterilization according to the following parameters or per instructions for use of the abutment if different.

METHOD	CONDITIONS	DRYING TIME
Moist Heat (Autoclave) Pre-Vacuum Displacement	132°C / (270°F) for 4 min	30 min
Moist Heat (Autoclave) Gravity Displacement	132°C / (270°F) for 15 min	30 min

Straumann North American Headquarters

Straumann USA, LLC
 60 Minuteman Road
 Andover, MA 01810
 Phone 800/448 8168 (US) • 800/363 4024 (CA)
 Fax 978/747 2490
 www.straumann.us • www.straumann.ca

ifu.straumann.com

© Straumann USA, LLC 2018. All rights reserved.

Straumann® and/or other trademarks and logos from Straumann® that are mentioned herein are the trademarks or registered trademarks of Straumann Holding AG and/or its affiliates. All rights reserved.