


Stage 4 | Aftercare and maintenance


# Step 1 Review visit




## Assessment and treatment planning

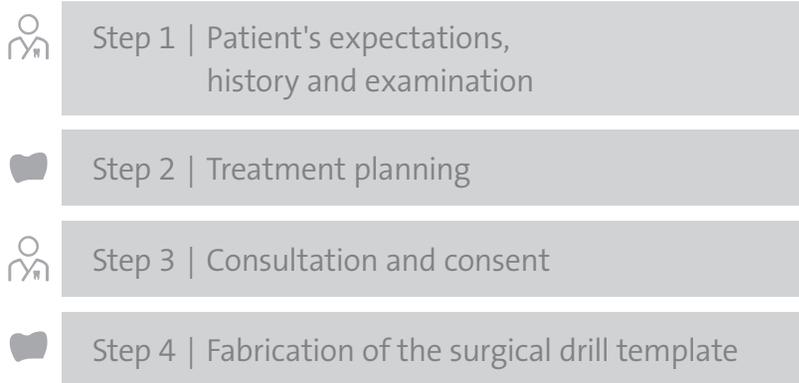


## Surgical procedures

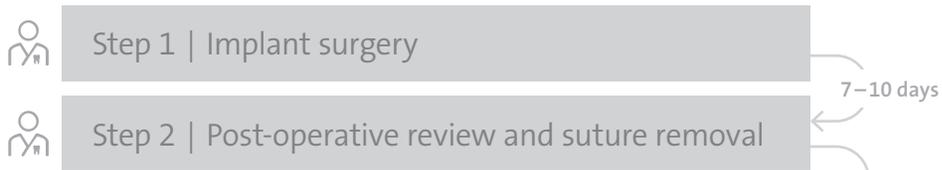

## Prosthetic procedures

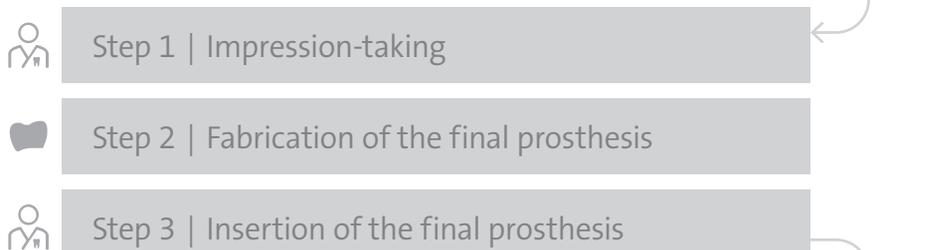

## Aftercare and maintenance

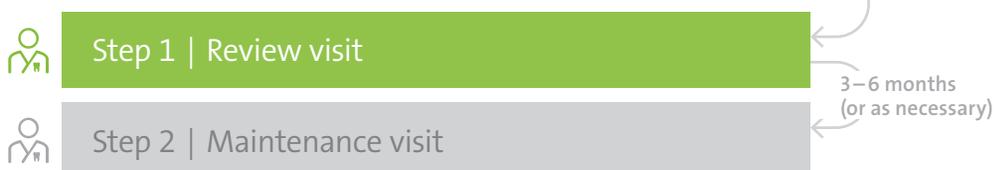

 In clinic with patient     Office / Lab work



## Contents

<b>Introduction</b>	<b>4</b>
<b>Learning objectives</b>	<b>4</b>
<b>1. Clinical examination and assessment</b>	<b>5</b>
1.1 Patient's feedback	5
1.2 Radiographic examination (if necessary)	5
1.3 What to check at the implant sites	6
<b>2. Final closure of the screw access holes for the screw-retained bridge</b>	<b>9</b>
2.1 Cleaning	9
2.2 Preparing	9
2.3 Closing	9
2.4 Bonding	10
2.5 Final filling and checking the occlusion	10
<b>3. Instructing the patient</b>	<b>11</b>
<b>4. Maintenance visits</b>	<b>11</b>
<b>Checklist for this visit</b>	<b>12</b>



## Introduction



The review visit with the patient should ideally take place **2 weeks** after the final prosthesis has been inserted. You can ask the patient about his or her experience with their new fixed dental prosthesis (FDP) and be able to assess if any further adjustments are required. In the case of a screw-retained final prosthesis, you can replace the temporary filling material with a permanent one if you and the patient are satisfied. This visit also gives the opportunity to reinforce optimal oral hygiene and care of the implant-borne restoration with the patient.

**Arrange to see the patient about 2 weeks after insertion of the final prosthesis to:**

- ask about the experience with the new FDP
- assess if adjustments are required
- place permanent fillings in a screw-retained FDP
- reinforce oral hygiene

## Learning objectives

-  Be able to examine and assess the condition of the FDP, the implants and the surrounding soft tissue.
-  Be able to assess the patient's oral hygiene compliance.
-  Be able to close the screw access holes permanently in the screw-retained FDP.
-  Be able to define individual recall intervals for the patient.



## 1. Clinical examination and assessment


### 1.1 Patient's feedback

Gather the patient's feedback about his or her oral comfort and function since the last visit.

### 1.2 Radiographic examination (if necessary)

If a radiograph of the implant sites was not taken immediately after the final restoration was placed, take a periapical radiograph during this visit with the long-cone paralleling technique. This radiograph will be the baseline for monitoring of future bone levels or any bony pathology.

Take a final baseline radiograph if necessary.

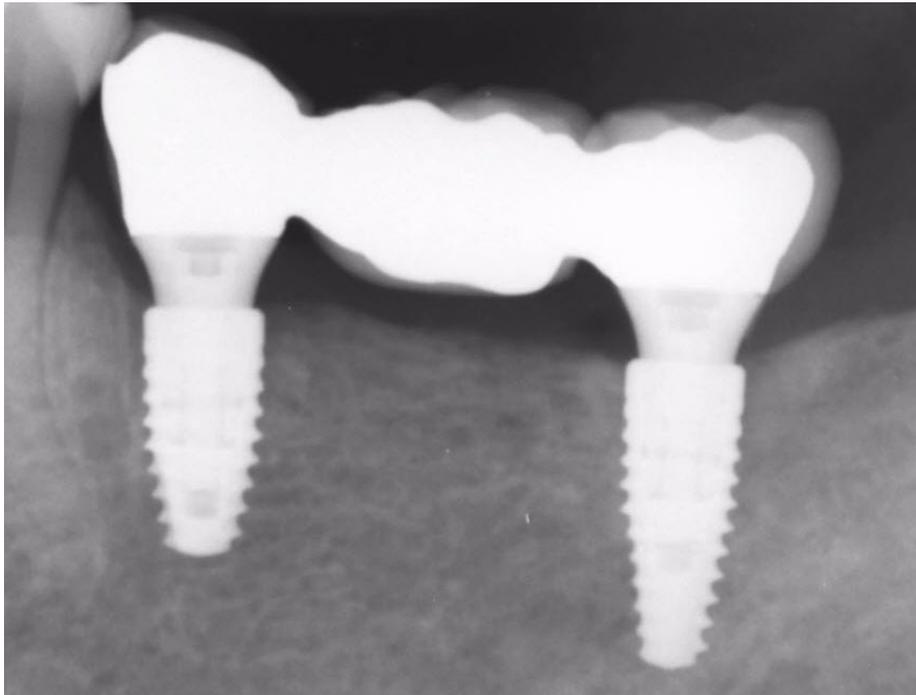



### 1.3 What to check at the implant sites

#### 1.3.1 Oral hygiene compliance and presence of plaque



Plaque monitoring should be performed and documented at every patient visit, to allow long-term monitoring of the patient's oral hygiene status. Plaque scores may be referenced when there is peri-implant mucositis and increased probing depths around implants.

Monitor plaque scores to reinforce oral hygiene.

#### 1.3.2 Clinical appearance of the peri-implant soft tissues



Take note of any swelling, bleeding or signs of infection such as suppuration. Monitor if there is a collar of at least **2 mm** of keratinized tissue around the implants.

Record the peri-implant soft tissue status.

#### 1.3.3 Clinical probing depths around the implants



Use a periodontal probe to record baseline clinical probing depths at this first review visit. Probing depths for conventionally placed implants, with supra-osseous implant platforms, generally range between **2 and 4 mm** if the tissues are healthy. Implants placed at bone level or at an infra-osseous level may exhibit slightly greater clinical probing depths.

Monitor peri-implant probing depths.

**⚠ Caution:** If the emergence profile of the suprastructure is wider than the implants, it may be difficult to assess probing depths due to the angulation of the probe.

#### 1.3.4 Bleeding on probing




The absence of bleeding on probing represents stability of the peri-implant soft tissues<sup>1,2</sup>. A probing force of **0.15 N** will help to avoid false positive readings for bleeding on probing around oral implants<sup>3</sup>.

Monitor any bleeding on probing sites.



### 1.3.5 Marginal fit between the implants and the FDP

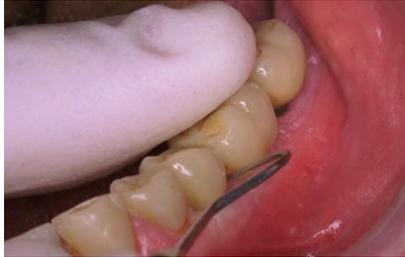

This can be assessed by using a dental explorer or if necessary take a periapical radiograph.

Check marginal fit of the prosthesis.



Possible causes of poor marginal fit are:

- Overly tight contact point on either the mesial or distal side.
- Too much soft tissue pressure from the peri-implant tissue, leading to incorrect seating of the final prosthesis.
- Over-contour of the prosthesis, causing too much soft tissue pressure.
- Inaccurate impression-taking.
- Inaccurate lab processes during prosthesis fabrication.

### 1.3.6 Stability of the FDP



Check for any signs of de-cementation or unwanted movement of the prosthesis.

Check for any decementation or unwanted instability of the prosthesis.

### 1.3.7 Patient's occlusion



The occlusal status of the implants and the FDP must be evaluated on a routine basis. Occlusal overload can cause loosening of the abutment screw(s) and prosthetic failure. Any signs of occlusal disharmony, such as premature contacts or interference should be identified and corrected to prevent occlusal overload.

Check for any signs of occlusal overload or disharmony.



# Aftercare and maintenance

Step 1 | Review visit

Clinical  
examination and  
assessment



- Check for only light centric contact, and no contact on lateral excursions.
- Check for any premature contacts.
- Is there anterior and lateral guidance with the natural dentition only?



Check that the occlusion only holds shimstock when the teeth are clenched hard.





## 2. Final closure of the screw access holes for the screw-retained bridge

### 2.1 Cleaning

Remove the temporary filling material and cotton pellets. Clean and dry the screw access holes thoroughly.



Prepare the screw access holes for permanent closure.

### 2.2 Preparing



Depending on the material of the screw-retained bridge and the choice of the restorative material to close the screw access holes, follow the cement or restorative material manufacturer's guidelines on conditioning or preparation of the screw access holes.

### 2.3 Closing



Close  $\frac{2}{3}$  of the screw access holes with a cotton pellet and Polytetrafluorethylene (PTFE) tape or sealing compound (e.g., gutta-percha).

Close  $\frac{2}{3}$  of the screw access holes with cotton and PTFE or sealing compound.



# Aftercare and maintenance

Step 1 | Review visit

Final closure  
of the screw  
access holes



## 2.4 Bonding



Apply the recommended bonding agent according to the instructions for use of the composite resin manufacturer's guidelines.

## 2.5 Final filling and checking the occlusion

Cover the upper 1/3 of the screw access holes with a composite resin restoration. Check the occlusion and grind down if necessary.



Restore the upper 1/3 of the screw access holes with the final filling material. Check the occlusion.



[Video: Final closure of the screw access holes for a screw-retained bridge](#)





### 3. Instructing the patient

Reinforce oral hygiene instructions and motivate the patient to take care of his or her new implant restoration.



Reinforce oral hygiene instructions with the patient.

 [Video: Review visit - 2 weeks after the insertion of the final prosthesis](#)



### 4. Maintenance visits

Decide on the appropriate recall frequency depending on the patient's risk factors (such as periodontitis and smoking), motivation, oral hygiene and peri-implant health status. This could be between 3 to 6 months or once a year.

Arrange for regular maintenance visits with the patient.

 Patients with a higher risk of peri-implantitis (e.g., smokers, history of chronic periodontal disease, poor plaque control) should be identified and monitored at least every 3 months.

Monitor patients who are at higher risk of peri-implant complications more frequently.



## CHECKLIST FOR THIS VISIT:

- Check the patient's comfort and function with his or her new implant-supported restoration. A thorough check on the condition of the implant-supported FDP, the surrounding soft tissue, and occlusion must be made.
- A baseline radiograph may be taken to help in future monitoring.
- Close the screw access holes with permanent filling material if a screw-retained FDP is used.
- Reinforce and emphasize the importance of good oral hygiene with the patient.
- Arrange for an appropriate maintenance interval for an adequate follow-up with the patient.



# Aftercare and maintenance

Step 1 | Review visit

## REFERENCES

- 1 Luterbacher et al. Diagnostic characteristics of clinical and microbiological tests for monitoring periodontal and peri-implant mucosal tissue conditions during supportive periodontal therapy (SPT). *Clin Oral Implants Res.* 2000 Dec;11(6):521-9.
- 2 Lang et al. Absence of bleeding on probing. An indicator of periodontal stability. *J Clin Periodontol.* 1990 Nov;17(10):714-21.
- 3 Gerber et al. Bleeding on probing and pocket probing depth in relation to probing pressure and mucosal health around oral implants. *Clin Oral Impl Res.* 2009;20(1):75-8.



# Aftercare and maintenance

## Step 1 | Review visit

### DISCLAIMER

Straumann® Smart is a blended training and education program focused on the education of general dentists who want to become surgically active in the field of dental implantology. The program is limited to information pertaining to straightforward implant cases and focuses on a reduced portfolio of products that are suitable for the treatment of such cases.

All clinical Straumann® Smart content – such as texts, medical record forms, pictures and videos – was created in collaboration with Prof. Dr. Christoph Hämmerle, Prof. Dr. Ronald Jung, Dr. Francine Brandenburg-Lustenberger and Dr. Alain Fontolliet from the University of Zürich, Clinic for Fixed and Removable Prosthodontics and Dental Material Science, Switzerland.

Straumann does not give any guarantee that Straumann® Smart provides sufficient knowledge or instruction for the dental professional to become surgically active in the field of implantology. It is the dental professional's sole responsibility to ensure that he/she has the appropriate knowledge and instruction before placing dental implants.

Straumann® Smart does not replace a careful and thorough analysis of each individual patient by a dental professional. Further, it does not imply any guarantee or warranty with regard to completeness of the information provided to the patient. It does not replace the dental professional's duty to inform the patient about the treatment, the products and the risks involved and to receive the patient's informed consent. The dental professional is solely responsible for determining whether or not a treatment or product is suitable for a particular patient and circumstances. Knowledge of dental implantology and instruction in the handling of the relevant products is always necessary and the sole responsibility of the dental professional. The dental professional must always comply with the individual product's Instructions For Use as well as all laws and regulations.

STRAUMANN DISCLAIMS, TO THE EXTENT POSSIBLE BY LAW, ANY LIABILITY, EXPRESS OR IMPLIED, AND BEARS NO RESPONSIBILITY FOR ANY DIRECT, INDIRECT, PUNITIVE, CONSEQUENTIAL OR OTHER DAMAGES, ARISING OUT OF OR IN CONNECTION WITH ANY INFORMATION PROVIDED TO PATIENTS, ERRORS IN PROFESSIONAL JUDGMENT, IN PRODUCT CHOICES OR PRACTICE IN THE USE OR INSTALLATION OF STRAUMANN PRODUCTS.

All clinical content as well as clinical and radiographic images are provided by courtesy of Prof. Dr. Christoph Hämmerle, Prof. Dr. Ronald Jung, Dr. Francine Brandenburg-Lustenberger and Dr. Alain Fontolliet from the University of Zürich, Clinic for Fixed and Removable Prosthodontics and Dental Material Science, Switzerland.

### **International Headquarters**

Institut Straumann AG  
Peter Merian-Weg 12  
CH-4002 Basel, Switzerland  
Phone +41 (0)61 965 11 11  
Fax +41 (0)61 965 11 01  
[www.straumann.com](http://www.straumann.com)

© Institut Straumann AG, 2016. All rights reserved.

Straumann® and/or other trademarks and logos from Straumann® mentioned herein are the trademarks or registered trademarks of Straumann Holding AG and/or its affiliates.