


Smart Product Descriptions


LOCATOR®

The LOCATOR® Implant Attachment System is intended for use with removable hybrid dentures that are retained solely by endosteal implants in the mandible or maxilla*.

The LOCATOR® abutments are made out of TAV and are available in various heights.

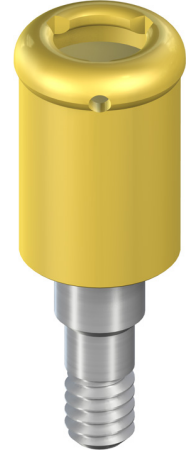

Implant line	Connection	Abutment heights
Standard Plus	NNC	1 mm 2 mm 3 mm
Bone Level Tapered	RC	4 mm 5 mm 6 mm
Bone Level Tapered	NC	2 mm 3 mm 4 mm 5 mm 6 mm

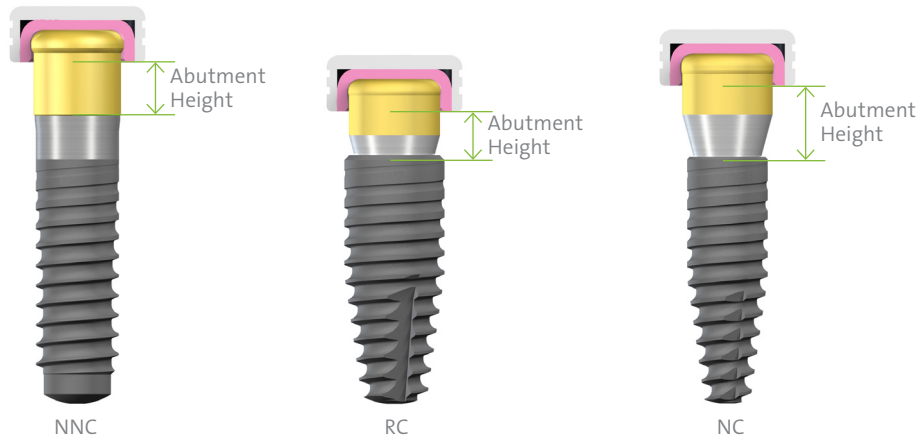

Contraindications

The LOCATOR® components

- are not suitable for combined tooth- and implant-supported dentures.
- cannot be used with implant divergences greater than 40°.

* Please note that Straumann® Smart Arch does not cover any LOCATOR® restorations in the maxilla.

Smart Product Descriptions

Characteristics of the LOCATOR® components

- With the LOCATOR® components you can accommodate up to 40° divergence between two implants.


Implant divergence up to 10° for a single implant

Color	Retention
● blue	0.68 kg
● pink	1.36 kg
● clear	2.27 kg

Implant divergence between 10° and 20° for a single implant

Color	Retention
● gray	0.0 kg
● red	0.45 kg
● orange	0.91 kg
● green	1.82 kg

- Even where occlusal space is limited, restorations in edentulous patients are possible thanks to the small vertical dimension of the LOCATOR® components.

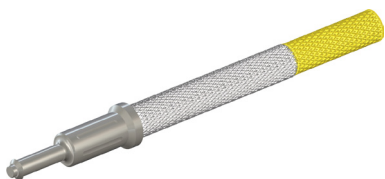







- With the help of the LOCATOR® Core Tool you can easily place and remove the LOCATOR® Retention Inserts.






- The self-locating design of the LOCATOR® components allows your patients to easily seat their dentures.
- An optimal connection between LOCATOR® abutments and denture is provided by dual retention.
- LOCATOR® components have an excellent long-term performance due to the high wear resistance of the parts.

Smart Product Descriptions







For Straumann® Standard Plus Narrow Neck CrossFit® (NNC) Implants

Titanium Abutments				
Art.-No.		Article	Dimensions	Material
048.581		NNC LOCATOR® Abutment	height 1 mm	TAV
048.582			height 2 mm	
048.583			height 3 mm	
048.584			height 4 mm	
048.585			height 5 mm	
048.586			height 6 mm	



For Straumann® Bone Level Tapered Narrow CrossFit® (NC) Implants

Titanium Abutments				
Art.-No.		Article	Dimensions	Material
022.2502		NC LOCATOR® Abutment	height 2 mm	TAV
022.2503			height 3 mm	
022.2504			height 4 mm	
022.2505			height 5 mm	
022.2506			height 6 mm	

For Straumann® Bone Level Tapered Regular CrossFit® (RC) Implants

Titanium Abutments				
Art.-No.		Article	Dimensions	Material
022.4501		RC LOCATOR® Abutment	height 1 mm	TAV
022.4502			height 2 mm	
022.4503			height 3 mm	
022.4504			height 4 mm	
022.4505			height 5 mm	
022.4506			height 6 mm	

For Straumann® Standard Plus NNC & Bone Level Tapered NC/RC Implants

Impression-taking/Master Cast Fabrication				
Art.-No.		Article	Dimensions	Material
048.197V4		LOCATOR® Impression Coping	height 4 mm, packaging 4 pieces	Al housing with LDPE insert
025.0120-04		LOCATOR® Female Analog	length 10 mm, Ø 4 mm, packaging 4 pieces	Al

Smart Product Descriptions

For Straumann® Standard Plus NNC & Bone Level Tapered NC/RC Implants

Art.-No.	Article	Description/Dimensions	Material
Lab Set, up to 20° Divergence Compensation			
048.189V2	 LOCATOR® Male Processing Package	includes: Denture Cap (∅ 5.5 mm, height 2.5 mm) with black Processing Male (height 1.9 mm), Block-out Spacer (048.196), clear Replacement Male (048.190), pink Replacement Male (048.191), blue Replacement Male (048.192), packaging 2 pieces	Ti/Nylon/LDPE
048.190V4	 LOCATOR® Replacement Male	clear, angle 0°–10°, height 1.7 mm, packaging 4 pieces	Nylon
048.191V4		pink, light retention, angle 0°–10°, height 1.7 mm, packaging 4 pieces	
048.192V4		blue, extra-light retention, angle 0°–10°, height 1.7 mm, packaging 4 pieces	
Lab Set, up to 40° Divergence Compensation			
048.182V2	 LOCATOR® Male Processing Package	extended range, includes: Denture Cap (∅ 5.5 mm, height 2.5 mm) with black Processing Male (height 1.9 mm), Block-out Spacer (048.196), green Replacement Male (048.193), orange Replacement Male (048.188), red Replacement Male (048.194), packaging 2 pieces	Ti/Nylon/LDPE
048.193V4	 LOCATOR® Replacement Male	green, extended range, angle 10°–20°, height 1.7 mm, packaging 4 pieces	Nylon
048.188V4		orange, light retention, extended range, angle 10°–20°, height 1.7 mm, packaging 4 pieces	
048.194V4		red, extra-light retention, extended range, angle 10°–20°, height 1.7 mm, packaging 4 pieces	
048.181V4		gray, extended range, zero retention, height 1.7 mm, packaging 4 pieces	
Tools and Auxiliary Parts			
048.199V4	 LOCATOR® Parallel Post	length 8 mm, packaging 4 pieces	LDPE
048.195V4		height 1.9 mm, packaging 4 pieces	
048.196V20	 LOCATOR® Block-out Spacer	thickness 0.4 mm, packaging 20 pieces	Silicone rubber
048.218V4	 LOCATOR® Processing Spacer	packaging 4 pieces	POM
046.413V4	 LOCATOR® Abutment Holder Sleeve	to fasten abutment to the tool, packaging 4 pieces	PSU
Tools and Auxiliary Parts			
046.415	 LOCATOR® Core Tool	three-part, length 100 mm	Stainless steel
046.416	 LOCATOR® Screwdriver	for Ratchet, short, length 15 mm	
046.417		for Ratchet, long, length 21 mm	
048.200	 LOCATOR® Angle Measurement Guide	length 50 mm, width 15 mm	

Al = Aluminum
 LDPE = Low-density polyethylene
 POM = Polyoxymethylene

PSU = Polysulfone
 TAV = Titanium-aluminum-vanadium alloy
 Ti = Titanium

Smart Product Descriptions

DISCLAIMER

Straumann® Smart is a blended training and education program focused on the education of general dentists who want to become surgically active in the field of dental implantology. The program is limited to information pertaining to straightforward implant cases and focuses on a reduced portfolio of products that are suitable for the treatment of such cases.

All clinical Straumann® Smart content – such as texts, medical record forms, pictures and videos – was created in collaboration with Prof. Dr. Christoph Hämmerle, Prof. Dr. Ronald Jung, Dr. Francine Brandenburg-Lustenberger and Dr. Alain Fontolliet from the University of Zürich, Clinic for Fixed and Removable Prosthodontics and Dental Material Science, Switzerland.

Straumann does not give any guarantee that Straumann® Smart provides sufficient knowledge or instruction for the dental professional to become surgically active in the field of implantology. It is the dental professional's sole responsibility to ensure that he/she has the appropriate knowledge and instruction before placing dental implants.

Straumann® Smart does not replace a careful and thorough analysis of each individual patient by a dental professional. Further, it does not imply any guarantee or warranty with regard to completeness of the information provided to the patient. It does not replace the dental professional's duty to inform the patient about the treatment, the products and the risks involved and to receive the patient's informed consent. The dental professional is solely responsible for determining whether or not a treatment or product is suitable for a particular patient and circumstances. Knowledge of dental implantology and instruction in the handling of the relevant products is always necessary and the sole responsibility of the dental professional. The dental professional must always comply with the individual product's Instructions For Use as well as all laws and regulations.

STRAUMANN DISCLAIMS, TO THE EXTENT POSSIBLE BY LAW, ANY LIABILITY, EXPRESS OR IMPLIED, AND BEARS NO RESPONSIBILITY FOR ANY DIRECT, INDIRECT, PUNITIVE, CONSEQUENTIAL OR OTHER DAMAGES, ARISING OUT OF OR IN CONNECTION WITH ANY INFORMATION PROVIDED TO PATIENTS, ERRORS IN PROFESSIONAL JUDGMENT, IN PRODUCT CHOICES OR PRACTICE IN THE USE OR INSTALLATION OF STRAUMANN PRODUCTS.

All clinical content as well as clinical and radiographic images are provided by courtesy of Prof. Dr. Christoph Hämmerle, Prof. Dr. Ronald Jung, Dr. Francine Brandenburg-Lustenberger and Dr. Alain Fontolliet from the University of Zürich, Clinic for Fixed and Removable Prosthodontics and Dental Material Science, Switzerland.

International Headquarters

Institut Straumann AG

Peter Merian-Weg 12

CH-4002 Basel, Switzerland

Phone +41 (0)61 965 11 11

Fax +41 (0)61 965 11 01

www.straumann.com

© Institut Straumann AG, 2016. All rights reserved.

Straumann® and/or other trademarks and logos from Straumann® mentioned herein are the trademarks or registered trademarks of Straumann Holding AG and/or its affiliates.